



Robert J Giraud
<Robert.J.Giraud@US
A.dupont.com>

03/01/04 12:55 PM

To: Rich Leukroth/DC/USEPA/US@EPA
cc: John Blouin/DC/USEPA/US@EPA, Greg Fritz/DC/USEPA/US@EPA,
david.menotti@shawpittman.com, Stephen H Korzeniowski
<Stephen.H.Korzeniowski@USA.dupont.com>, Robert C Buck
<Robert.C.Buck@USA.dupont.com>, bill.beers@omnova.com

Subject: revisions to final draft ECA appendices based on today's drafting
committeecall

Colleagues,

Thank you for your comments on the appendices during this morning's call.

Here is revised Telomers Appendix A.4. Per the discussion (to prevent confusion with the new text for Part IX of the ECA cover document, the word "assembling" is changed to "receiving" on line 4 of page A.4-2. Similarly, I have revised the title of Section 4.1 (of Appendix A.4 for telomers) from "Assembly of Components" to "Handling of Components" for the same reason.

(See attached file: App A.4 telomers incin test draft 2-27-04-revised.pdf)

Here is revised Fluoropolymers Appendices A.2 through A.4. I have corrected errant mention of Composite 21 to Composite 1 in line 4 of page A.4-2 of fluoropolymers appendix A.4

(See attached file: App A.2 through A.4 Fluoropolymers draft 2-27-04-revised.pdf)

Here is revised compiled Appendices B through G. Since I had forgotten to introduce Appendix E.3 in the opening of Appendix C.2 and based on this morning's discussion, please see new section C.2.5.6 introducing Appendix E.3. Also, please see revised Appendix E.3 based on this morning's discussion. Please note that the parentheticals for "provided Phase II is performed" is to clarify that there will be no report for Phase II incineration testing if Phase II is not carried out (e.g., need for Technical Consultation and no agreement to proceed with Phase II testing) and to clarify that the test substance composites are germane only to Phase II and not to Phase I. I have also corrected an oversight on Friday and have bolded the docket number in the title section of the second page (Fluoropolymers) of Appendix G. Furthermore, I have added a cross-reference to Appendix C.2.5 in the last paragraph of Appendix C.1.3 (line 8 of page C.1- 4) with regard to reporting results for improved clarification.

(See attached file: Appendices B through G draft 2-27-04-revised.pdf)

If you have any questions or comments, please let me know.

I look forward to our 9 am to 10:30 am call on Tuesday March 2.

Best Regards,

Robert Giraud

This communication is for use by the intended recipient and contains information that may be privileged, confidential or copyrighted under applicable law. If you are not the intended recipient, you are hereby formally notified that any use, copying or distribution of this e-mail, in whole or in part, is strictly prohibited. Please notify the sender

by return e-mail and delete this e-mail from your system. Unless explicitly and conspicuously designated as "E-Contract Intended", this e-mail does not constitute a contract offer, a contract amendment, or an acceptance of a contract offer. This e-mail does not constitute a consent to the use of sender's contact information for direct marketing purposes or for transfers of data to third parties.

Francais Deutsch Italiano Espanol Portugues Japanese Chinese Korean

http://www.DuPont.com/corp/email_disclaimer.html



App A.4 telomers incin test draft 2-27-04-reviser App A.2 through A.4 Fluoropolymers draft 2-27-04-reviser



Appendices B through G draft 2-27-04-revised

1 **APPENDIX A.2**2 **RATIONALE FOR SELECTING COMPOSITES TO BE TESTED**

3

4 Review of Figure A.2-1 demonstrates that fluoropolymers
5 industry products can be divided into 3 broad categories as
6 follows:

7

- 8 • Dry melt resins
- 9 • Dry non-melt resins and gums
- 10 • Aqueous dispersions

11

12 These three broad categories can in turn be divided into
13 four representative classes as follows:

14

- 15 • Dry melt resins
 - 16 1. FEP, PFA, THV, ETFE, HTE
- 17
- 18 • Dry non-melt resins and gums
 - 19 2. Dry non-melt resins
 - 20 3. Fluoroelastomers (dry non-melt gums)


21

- 22 • Aqueous dispersions
 - 23 4. PTFE, FEP, PFA, THV

24

25 Composite samples of each of these four representative
26 classes were selected as the test substance for this
27 testing program in order to represent the entire range of
28 fluoropolymers involved.

Figure A.2-1. Fluoropolymer Industry Overview

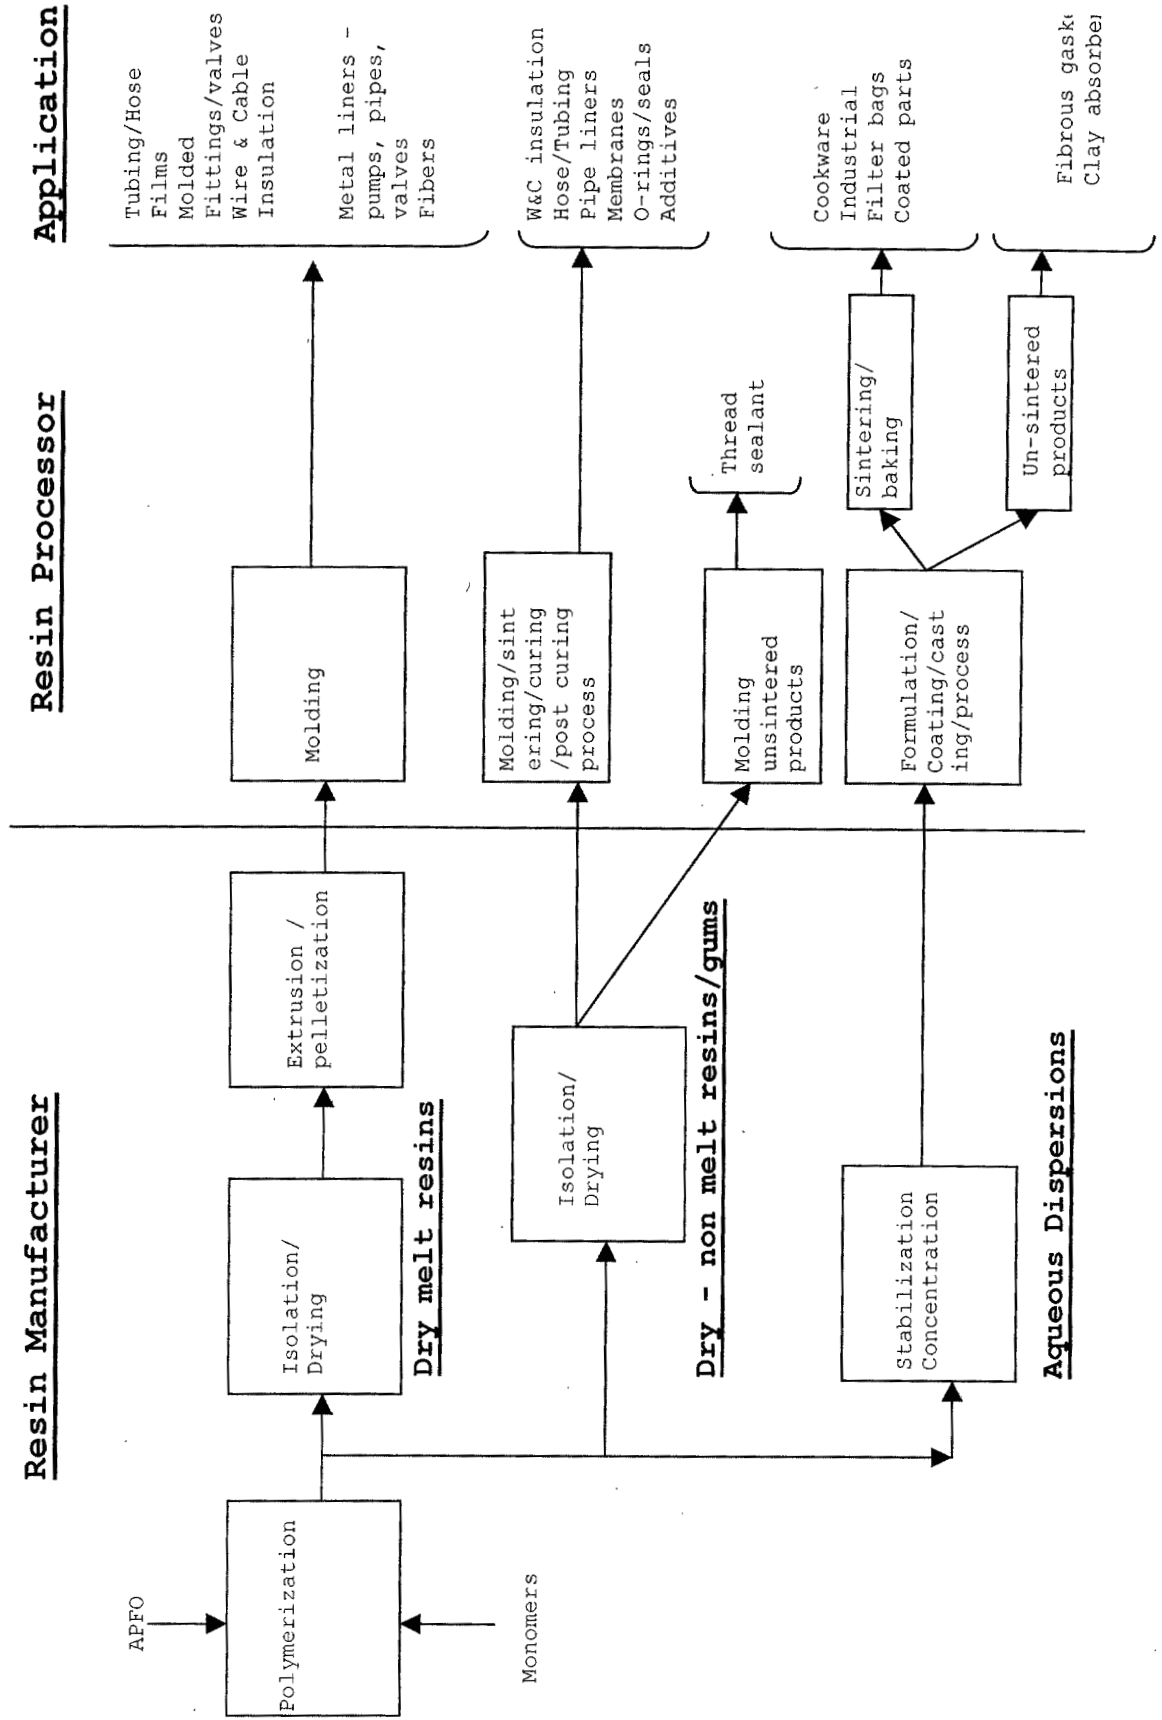

1 **APPENDIX A.3**2 **COMPOSITION OF COMPOSITES TO BE TESTED**

3
4 The four composite test substances for this test program
5 are presented below in Table A.3-1 with the fluoropolymer
6 types, CAS numbers, and associated monomers for these
7 fluoropolymers. Each fluoropolymer used in each relevant
8 test substance composite will have been made using APFO.
9

10 **Table A.3-1. Test Substance Composites by Type**

Test Substance	Fluoropolymer Type	CAS Number	Associated Monomers	
Composite 1 - Dry non-melt resin	PTFE	9002-84-0	TFE	
	Modified PTFE	26655-00-5	TFE, PPVE	
Composite 2 - Dry melt resins	FEP	25067-11-2	TFE, HFP	
	PFA	26655-00-5	TFE, PPVE	
		31784-04-0	TFE, PEVE	
	THV	25190-89-0	TFE, HFP, VDF	
	ETFE	68258-85-5	TFE, E	
HTE	35560-16-8	TFE, HFP, E		
Composite 3 - Fluoroelastomers Copolymers	Fluoroelastomer	9011-17-0	VDF, HFP	
	Copolymers	Fluoroelastomer	25190-89-0	TFE, HFP, VDF
		Terpolymers		
	Base resistant elastomers	54675-89-7,	TFE, VDF, P	
		27029-05-6	TFE, P	
	Perfluoroelastomers	26425-79-6	TFE, PMVE	
CTFE elastomers	9010-75-7	CTFE, VDF		
Low temperature elastomers	CBI	TFE, VDF		
Composite 4 - Aqueous Dispersions	PTFE	9002-84-0	TFE	
	FEP	25067-11-2	TFE, HFP	
	PFA	26655-00-5	TFE, PPVE	
		31784-04-0	TFE, PEVE	
THV	25190-89-0	TFE, HFP, VDF		

11
12 Confidential business information (CBI) regarding the
13 chemical identity of Low temperature elastomers has been
14 submitted to EPA under separate cover.

1 **APPENDIX A.4**2 **PREPARATION OF COMPOSITES TO BE TESTED**3
4 4.1 Approach

5
6 A composite mixture of representative fluoropolymers, as
7 solids, will be prepared for each of the four test
8 substance composites.

9
10 The polymer samples will be first quality product polymer,
11 substantially free of inorganic constituents. Each sample
12 will be from a representative grade for each applicable
13 fluoropolymer type from each applicable company.

14
15 A hypothetical example for Composite Z in Table A.4-1 below
16 shows how the composites will be assembled. In this
17 example with 4 types across 4 companies, there are 11 x's.
18 Hence, composite Z would be made up of 11 equal proportions
19 of the materials indicated with an x.

20
21 **Table A.4-1. Example for Compositing Across Companies & Types**

Test Substance	Fluoropolymer Type	Company A	Company B	Company C	Company D
Composite Z	Type 1		x	x	x
	Type 2	x	x	x	x
	Type 3			x	
	Type 4	x	x	x	

22
23 4.2 Preparation

24
25 Representative samples of each component from each
26 applicable company for each composite will be sent to the
27 compositing facility(ies) in packaging customarily used for
28 product sample packaging or in polyethylene, polypropylene,
29 or glass containers.

30
31 Each composite will be prepared under conditions designed
32 to prevent cross-contamination and designed to assure
33 solids temperatures less than or equal to 60 °C.

34
35 Following preparation of each composite, the composite will be
36 placed in a polyethylene, polypropylene, or glass container.

37
38 4.2.1 Composite 1

39
40 Dry non-melt resins are available in powder form. Equal

1 weights of the powder form of each of the two types of
2 components (following the approach in the example for
3 Composite Z in Section 4.1 above) will be mixed together in
4 dry form to yield Composite 1.

5
6 4.2.2 Composite 2

7
8 FEP, PFA, THV, ETFE, and HTE dry melt resins are available
9 in powder form. Equal weights of the powder form of each
10 component (following the approach in the example for
11 Composite Z in Section 4.1 above) will be mixed together in
12 dry form to yield Composite 2.

13
14 4.2.3 Composite 3

15
16 Fluoroelastomers are available in slab, lump, or sheet
17 form. Composite 3 will be prepared following one of the
18 following approaches:

19
20 a) Equal weights of each component (following the approach
21 in example for Composite Z in Section 4.1) will be mixed
22 on a rubber mill to produce a homogenous slab of preset
23 thickness to yield Composite 3.

24
25 Or

26
27 b) Each component of Composite 3 will be cryogenically
28 cooled (to make the elastomers brittle) and size-reduced
29 (e.g., ground) to produce powder. Equal weights of the
30 powder form of each component (following the approach in
31 the example for Composite Z in Section 4.1) will be mixed
32 together in dry form to yield Composite 3.

33
34 4.2.4 Composite 4

35
36 Aqueous dispersions of PTFE, FEP, PFA, and THV are
37 available as dispersions containing 20 to 60% fluoropolymer
38 solids by weight. Composite 4 will be prepared following
39 one of the following approaches:

40
41 a) Equal weights (on a dry solids basis) of each component
42 in aqueous dispersion form (following the approach in
43 example for Composite Z in Section 4.1) will be mixed
44 together in liquid form. Solids will be separated from
45 the resulting liquid composite to yield low water content
46 (i.e., drip free) fine solids.

1

2

Or

3

4

b) Solids will be separated from liquid for each component of Composite 4 to yield low water content (i.e., drip free) fine solids for each component. Equal weights of the solids from each component (following the approach in the example for Composite Z in Section 4.1) will be mixed together to yield Composite 4.

10

11

4.3 Verification

12

13

14

15

16

17

18

19

20

21

22

23

24

25

26

27

28

In order to assure that composite samples in this testing program have been made up of clearly identified materials, the preparation of the composites will include formal Chain of Custody procedures. A chain of custody form will be included with each component material going into the composite to show the identity of the component material and each transfer of custody from its point of origination to preparation of the composite.

Once prepared, each composite will be accompanied by a new chain of custody until it reaches the incineration testing facility.

For documentation, the facility preparing a given composite will generate a report to be submitted to EPA with the final report for Phase II incineration testing.

1 **APPENDIX B.1**
2 **GUIDELINE FOR THERMOGRAVIMETRIC ANALYSIS**
3

4 ASTM E 1868-02 "Standard Test Method for Loss-On-Drying by
5 Thermogravimetry" will be used as the guideline for conducting
6 the analysis described in Appendix C.2.3 with the following
7 modifications for this testing program:
8

Section	Modification
2.1	<ul style="list-style-type: none"> Standard practices at the University of Dayton Research Institute (UDRI) may be used as references throughout the standard in place of the ASTM standards noted in this section.
4.1	<ul style="list-style-type: none"> The loss-on-drying value specified in the second through fifth sentences of this section will not be recorded.
7.1.3	<ul style="list-style-type: none"> The programming rate of the furnace will be set at 10 to 25°C/min, rather than 5°C/min. Pursuant to section 11.6, the temperature program rate will be documented in the report. The isothermal temperature within the range of 25 to 1000°C will be maintained $\pm 3^\circ\text{C}$, rather than $\pm 2^\circ\text{C}$.
7.1.4	<ul style="list-style-type: none"> The specimen atmosphere control system will be capable of supplying dry air in addition to "inert dry gas (usually purified grade nitrogen)".
7.1.7	<ul style="list-style-type: none"> The temperature program rate will be set at 10 to 25°C/min, rather than 5°C/min. Pursuant to section 11.6, the temperature program rate will be documented in the report. The temperature program rate will be controlled to within the range of $\pm 3^\circ\text{C}/\text{min}$, rather than $\pm 0.1^\circ\text{C}/\text{min}$. Within the range of 25 to 1000°C, the isothermal temperature will be maintained within $\pm 3^\circ\text{C}$, rather than $\pm 2^\circ\text{C}$.
11.4	<ul style="list-style-type: none"> The mass of the test specimen noted in the first sentence of this section will be 0.005 to 5 mg, rather than 10 ± 1 mg (i.e., 9 to 11 mg).
11.6	<ul style="list-style-type: none"> The test specimen heating rate will be set at 10 to 25°C/min, rather than 5°C/min noted in the first sentence of this section. Pursuant to section 11.6, the temperature program rate will be documented in the report.
11.9	<ul style="list-style-type: none"> Termination criteria will follow Test Method A as outlined in section 11.10.1.

11.10.1	<ul style="list-style-type: none">• The "fixed period of test time" mentioned in this section will be set at 5 min.
11.10.1.1	<ul style="list-style-type: none">• Loss-on-drying values will not be recorded.
12.1	<ul style="list-style-type: none">• The loss-on-drying value will not be calculated.
13.1.1	<ul style="list-style-type: none">• The "identification and description of the material being tested" will be consistent with the information known to the analyst.
13.1.5	<ul style="list-style-type: none">• The loss-on-drying value will not be included in the report.
14.2	<ul style="list-style-type: none">• This section is not applicable because the Test Method A termination criteria will be used.

9
10
11
12
13
14
15
16
17

Reference

ASTM E 1868-02 "Standard Test Method for Loss-On-Drying by Thermogravimetry", ASTM International. For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For Annual Book of ASTM Standards volume information, refer to the standard's Document Summary page on the ASTM website.

1 **APENDIX C.1**2 **PFOA TRANSPORT TESTING**3
4 C.1.1 Significance

5
6 Testing will be performed to verify that potential PFOA
7 emissions from the combustion testing described in Appendix
8 C.2 can be quantitatively transported from the high
9 temperature reactor into the exhaust gas sampling apparatus
10 (aqueous solution bubblers).

11
12 Acceptable PFOA transport will be demonstrated if the
13 transport efficiency (as computed in one or more of the
14 formulas below) is greater than or equal to 70%.

15
16 C.1.2 Experimental Plan17
18 C.1.2.1 Base Plan

19
20 Transport of PFOA across the laboratory-scale thermal
21 reactor system described in Appendix C.2.4 and into the
22 exhaust gas bubblers described in Appendix D.1 will be
23 quantitatively determined as an indication of transport
24 from the high temperature reactor into the bubblers.

25
26 A PFOA standard of known purity greater than or equal to
27 97% will be gasified at 150 to 250 °C (based on
28 thermogravimetric analysis of PFOA) with transfer line and
29 reactor temperatures 0 to 100 °C higher than the
30 gasification temperature.

31
32 Three replicate transport efficiency test runs will be
33 conducted. A minimum of one blank run will be conducted
34 prior to each transport efficiency test run.

35
36 The sample size of the PFOA standard to be gasified will be
37 less than 5 mg. The reactor exhaust gas will be collected
38 into bubbler aqueous solution as described in Appendix D.1
39 (including an HPLC water rinse of the flexible tubing [used
40 to connect the thermal reactor system and the bubbler
41 assembly] into the aqueous solution composite), which will
42 be analyzed for PFOA as described in Appendix D.2. In
43 order to provide a second way of demonstrating quantitative
44 transport, this aqueous solution composite will also be
45 analyzed for total fluorine as described in Appendix D.3.
46 (Testing for total fluorine is included due to possibility
47 of thermal degradation of PFOA under transport test

1 conditions.) Therefore, for this transport testing the
2 amount of PFOA fed to the thermal reactor system will be
3 sufficiently high to assure that the total fluorine input
4 to the thermal reactor system will be greater than 140% of
5 the mass corresponding to the limit of quantitation (LOQ)
6 for total fluorine in the aqueous solution composite. (The
7 LOQ for total fluorine in aqueous solution is much higher
8 than the LOQ for PFOA in aqueous solution.)
9

10 The amount of PFOA and total fluorine in the thermal
11 reactor system exhaust gas will be determined via analysis
12 of the aqueous solution composite as noted above.
13

14 The amount of PFOA fed to the thermal reactor system will
15 be known based on measurement prior to gasification and
16 will be verified by weighing the pyroprobe insert cartridge
17 before and after each test run. The amount of fluorine
18 input to the system will be calculated from the amount of
19 PFOA fed, the known purity of the PFOA, and the known
20 fluorine fraction of the PFOA standard.
21

22 PFOA transport efficiency (TE) as a percentage will be
23 computed as follows:
24

$$25 \quad \% \text{ PFOA TE} = \frac{\text{mass of PFOA in aqueous solution composite}}{\text{mass of PFOA fed to thermal reactor system}} * 100 \quad (1)$$

26
27

28 Total fluorine (TF) transport efficiency as a percentage
29 will be computed as follows:
30

$$31 \quad \% \text{ Total F TE} = \frac{\text{mass of total F in aqueous solution composite}}{\text{mass of total F fed to thermal reactor system}} * 100 \quad (2)$$

32
33

34 C.1.2.2 Contingent Testing

35

36 If the transport efficiencies for both PFOA (equation 1)
37 and total fluorine (equation 2) are less than or equal to
38 70%, then additional work will be performed. This
39 additional work will be performed in a step-wise fashion to
40 determine if consideration of one or more of the following
41 procedural revisions enables achievement of 70% transport
42 efficiency as follows:
43

44 Step 1. The flexible tubing between the thermal reactor
45 system and the bubbler assembly from the experiment
46 described in Section C.1.2.1 would be
47 quantitatively rinsed with methanol. This methanol
48 rinsate would be analyzed for PFOA (as described in

1 Appendix D.2) and/or for total fluorine (as
2 described in Appendix D.3). Revised transport
3 efficiency (TE) as a percentage for PFOA (equation
4 3) and/or total fluorine (equation 4) would be
5 computed by including the mass of analyte in the
6 methanol rinse in the numerator as follows:

$$7$$

$$8$$

$$9 \quad \% \text{ PFOA TE} = \frac{\text{mass}_{\text{PFOA out}}}{\text{mass}_{\text{PFOA in}}} * 100 \quad (3)$$

$$10$$

11

12 where $\text{mass}_{\text{PFOA out}}$ = mass of PFOA in bubbler
13 aqueous solution composite
14 + mass of PFOA in methanol
15 rinse

16

17 and $\text{mass}_{\text{PFOA in}}$ = mass of PFOA fed to thermal
18 reactor system

$$19$$

$$20$$

$$21 \quad \% \text{ Total F TE} = \frac{\text{mass}_{\text{total F out}}}{\text{mass}_{\text{total F in}}} * 100 \quad (4)$$

$$22$$

23

24 where $\text{mass}_{\text{total F out}}$ = mass of total F in
25 bubbler aqueous
26 solution composite
27 + mass of total F in
28 methanol rinse

29

30 and $\text{mass}_{\text{total F in}}$ = calculated mass of
31 total F in PFOA fed to
32 thermal reactor system

33

34 Step 2 (if necessary) The experiment described in Section
35 C.1.2.1 would be repeated with
36 reagent(s) (e.g. NaOH) added to the
37 bubbler aqueous solution to determine
38 if reagent addition enhances analyte
39 absorption, thereby improving transport
40 efficiency. Transport efficiency would
41 be calculated using equation (1) and/or
42 (2) above. The impact of reagent
43 addition on LOQ for PFOA analysis
44 described in Appendix D.2 would be
45 determined.

46 C.1.3 Reporting of Results

47

48

49 Following completion of PFOA transport testing as described
50 in this appendix and prior to beginning incineration
51 testing described in Appendix C.2, a letter report will be

1 submitted to EPA with the transport efficiency result(s)
2 and indication of what contingent testing, if any, was
3 performed.
4
5 If Appendix C.2 incineration testing is performed, the
6 detailed results of Appendix C.1 transport testing will be
7 included in the test report for Appendix C.2 incineration
8 testing described in Appendix C.2.5. If Appendix C.2
9 incineration testing is not performed, the detailed results
10 of Appendix C.1 transport testing will be provided in a
11 test report for Appendix C.1 transport testing.

1 **APPENDIX C.2**
2 **INCINERATION TESTING**

3
4 **C.2.1 ELEMENTAL ANALYSIS**

5
6 C.2.1.1 Introduction

7
8 Elemental analysis as described in Section C.2.1 will be
9 performed for each test substance composite to aid in
10 preparation for combustion testing described in Section
11 C.2.4.

12
13 As Kissa (1998) points out, technique strongly affects
14 analytical results for fluorinated organic compounds such
15 as fluorinated surfactants and fluorinated polymers due to
16 the carbon-fluorine bond:

17
18 Fluorine in organic compounds is usually
19 determined by converting organic fluorine to an
20 inorganic fluoride. Various combustion methods
21 are routinely used for this purpose. However,
22 the carbon-fluorine bond is exceptionally strong,
23 and extremely vigorous conditions are needed for
24 a quantitative mineralization. Conventional
25 combustion conditions used for the determination
26 of carbon and hydrogen in nonfluorinated organic
27 compounds are not adequate for a quantitative
28 analysis of fluorinated surfactants.

29
30 Therefore, total fluorine analysis will be performed using
31 "extremely vigorous conditions" as described in Section
32 C.2.1.2, and the commercially available conventional
33 technique used for empirical determination of carbon and
34 hydrogen content (described in Section C.2.1.3) will
35 provide estimated values.

36
37 C.2.1.2 Total Fluorine

38
39 Each test substance composite will be characterized via
40 analysis of total fluorine content.

41
42 Based on manufacturing process knowledge, the levels of
43 total fluorine in the components of test substance
44 composites are orders of magnitude higher than the
45 potential trace level of inorganic fluoride in these
46 materials. Therefore, for this test program, the total
47 organic fluorine value for each test substance composite

1 will be considered to be the same as the total fluorine
2 value.

3
4 Total fluorine content will be measured via the Wickbold
5 Torch method; see Appendix D.3.

6 7 C.2.1.3 Carbon and Hydrogen

8
9 In order to provide information for stoichiometric
10 calculations in Section C.2.2, the carbon and hydrogen
11 content of each test substance composite is needed. Based
12 on manufacturing process knowledge of the polymers in this
13 program, levels of sulfur, and nitrogen are expected to be
14 less than 0.1% and to thereby have negligible effect on
15 stoichiometric calculations.

16 17 C.2.1.3.1 Theoretical Determination

18
19 Where the elemental composition of a test substance
20 composite is known from the identity of the components in a
21 given composite, the carbon and hydrogen content of the
22 test substance composite can be calculated.

23
24 For example, where each of the components of a test
25 substance composite are polytetrafluoroethylene (PTFE), the
26 carbon and hydrogen can be determined knowing the molecular
27 formula for PTFE is $(C_2F_4)_n$ as follows:

28

	number	atomic weight	weight %
carbon (C)	2	12	24
hydrogen (H)	0	1	0
fluorine (F)	4	19	76
total			100

29 30 C.2.1.3.2 Empirical Determination

31
32 Where compositional information on carbon and hydrogen
33 content is not known from the identity of the components in
34 a given composite, each such test substance composite will
35 be analyzed for carbon and hydrogen.

36
37 As noted in Section C.2.1.1, empirical determination of
38 carbon in test substance composites via commercially
39 available conventional techniques is expected to
40 underestimate the carbon content of the test substance
41 composites due to the strength of the carbon-fluorine bond.
42 Similarly, empirical determination of hydrogen in test

1 substance composites via commercially available
2 conventional techniques is expected to overestimate the
3 hydrogen content of the test substance composites.

4
5 The carbon content of the test substance composite can be
6 measured by determining the carbon dioxide (CO₂) generated
7 by the oxidation of the sample. This oxidation may be
8 accomplished by high temperature combustion, catalytic
9 combustion, or wet chemical oxidation. The CO₂ is measured
10 directly by an infrared detector or a thermal conductivity
11 detector, via absorption into a suitable solution (e.g.,
12 potassium hydroxide) and gravimetric determination, or by
13 conversion to methane for measurement via a flame
14 ionization detector.

15
16 The hydrogen content of the sample can be determined by
17 difference with knowledge of the fluorine content and
18 carbon content of the sample where the moisture content and
19 chlorine content of the sample are negligible or known.
20 Alternatively, the hydrogen content of the sample is
21 measured by determining the water generated by high
22 temperature combustion of the sample. Measurement of water
23 in the combustion gas for this analysis may be accomplished
24 by techniques such as use of an infrared detector or
25 absorption on a dessicant with gravimetric determination.
26 With empirical hydrogen determination, it is important to
27 correct for the water in the combustion gas attributable to
28 the moisture content in the sample to obtain the hydrogen
29 content of the sample; see Section C.2.1.4.

30
31 Manufacturing process knowledge of the polymers will be
32 used to review the elemental analysis results and to form
33 the basis for interpreting non-detects. For example, if
34 the hydrogen analytical result for a perfluorinated polymer
35 is less than a quantitation limit of 0.1%, then the
36 analytical result will be replaced with 0.

37 38 C.2.1.4 Moisture

39
40 Where preparation (as described in Appendix A.4) for a
41 given test substance composite has involved dewatering, the
42 moisture (or solids) content of each such test substance
43 composite will be determined in order to provide a dry
44 basis for calculations as needed.

45
46 Moisture is determined by measuring the loss of weight of
47 the sample when heated under controlled conditions. A

1 representative sample is weighed and placed in a crucible
2 (or dish) and evaporated to dryness in an air or nitrogen
3 atmosphere at a defined temperature setpoint (e.g., 103 °C
4 to 105 °C) in the range of 100 °C to 125 °C. The moisture
5 value is calculated as the loss in weight (difference
6 between the starting weight of sample and the final weight
7 of sample) divided by the starting weight of sample.
8 Similarly, a solids value can be calculated as the final
9 weight of sample divided by the starting weight of sample.

11 C.2.2 COMBUSTION STOICHIOMETRY

13 Combustion stoichiometry calculations as described in
14 Section C.2.2 will be performed to aid in preparation for
15 combustion testing described in Section C.2.4

17 First, the weight percent values from Section C.2.1 are
18 converted to molar quantities on a dry basis.

20 Second, based on Chapter 3 of *Combustion Fundamentals for*
21 *Waste Incineration* (American Society of Mechanical
22 Engineers, 1974), the reaction products for these molar
23 quantities are calculated assuming complete combustion with
24 the following rules:

26 a) All carbon (C) in feed converts to carbon dioxide (CO₂)
27 $C + O_2 \rightarrow CO_2$

29 b) All sulfur (S) in feed converts to sulfur dioxide (SO₂)
30 $S + O_2 \rightarrow SO_2$


32 c) The halogens (Cl, F) in feed convert to hydrogen halides
33 $H_2 + Cl_2 \rightarrow 2HCl$
34 $H_2 + F_2 \rightarrow 2HF$

36 d) Hydrogen (H) present in feed in excess of that
37 required to yield products in item c) above will be
38 converted to water
39 $2H_2 + O_2 \rightarrow 2H_2O$

41 e) Nitrogen (N) from feed or air is emitted as molecular
42 nitrogen
43 $N_2 \rightarrow N_2$

45 Third, with these rules, the balanced chemical reaction for
46 combustion of a compound can be written.

1 For example, the resulting reaction equation for a
2 hydrocarbon like methane (CH₄) is



4
5 Note that the term feed in the preceding rules (a through
6 e) includes both material being combusted and the fuel
7 source of hydrogen such as methane or methanol.
8 Additionally, stoichiometric calculations as described
9 above presume that the compounds undergoing combustion are
10 essentially free of inorganic constituents.

11
12 These calculations provide the theoretical amount of oxygen
13 needed for the overall combustion reaction for the feed
14 based on the available information used in the
15 calculations. The initial estimate for the amount of
16 oxygen to be used in combustion testing will be determined
17 from this theoretical amount with adjustments for target
18 oxygen level in thermal reactor system exhaust gas. The
19 actual amount of oxygen to be used in combustion testing
20 will be based oxygen monitoring described in Section C.2.4.

21
22 These stoichiometric calculations will also be used as
23 needed to initially estimate and adjust experimental
24 conditions for combustion testing in Section C.2.4.

25

26 **C.2.3 THERMOGRAVIMETRIC ANALYSIS**

27

28 Thermogravimetric analysis (TGA) will be conducted to
29 determine the temperature range required for gasification
30 of each test substance composite. TGA will be conducted in
31 flowing air from room temperature to 1000°C as described in
32 Appendix B.1.

33

34 The TGA weight-loss profile for each test substance composite
35 will be evaluated to determine the temperature at which the
36 weight loss reaches a final asymptote across the temperature
37 range investigated. This temperature corresponds to the
38 point at which no further gasification (under test
39 conditions) occurs for the material and will be considered
40 the temperature for complete gasification of the material.

41

42 **C.2.4 Combustion Testing**

43

44 C.2.4.1 Test Objective

45

46 The objective of the testing program described in Appendix
47 C.2 is to assess the potential for waste incineration of

1 each test substance composite to emit PFOA, based on
2 quantitative determination of potential exhaust gas levels
3 of PFOA from laboratory-scale combustion testing under
4 conditions representative of typical municipal waste
5 combustor operations in the U.S.


6
7 C.2.4.2 Experimental Apparatus

8
9 Combustion testing will make use of the Advanced Thermal
10 Reactor System (ATRS) at the University of Dayton Research
11 Institute (UDRI). The ATRS is a laboratory-scale, non-
12 flame, batch-charged, continuous flow thermal reactor
13 system. The use of this non-flame thermal reactor system
14 gives a conservative representation of full-scale waste
15 incineration prior to air pollution controls.

16
17 In the ATRS, the test sample is gasified and transported to a
18 high temperature reactor. In the high temperature reactor,
19 the sample vapors are subjected to controlled conditions for
20 residence time and temperature. As described in Sections
21 C.2.4.5 and C.2.4.6, combustion products will be monitored or
22 collected for quantitative analysis.

23
24 A schematic of the ATRS as configured for this test program
25 is shown in Figure C.2-1.

26
27 **Figure C.2-1. Schematic of ATRS for this Test Program**

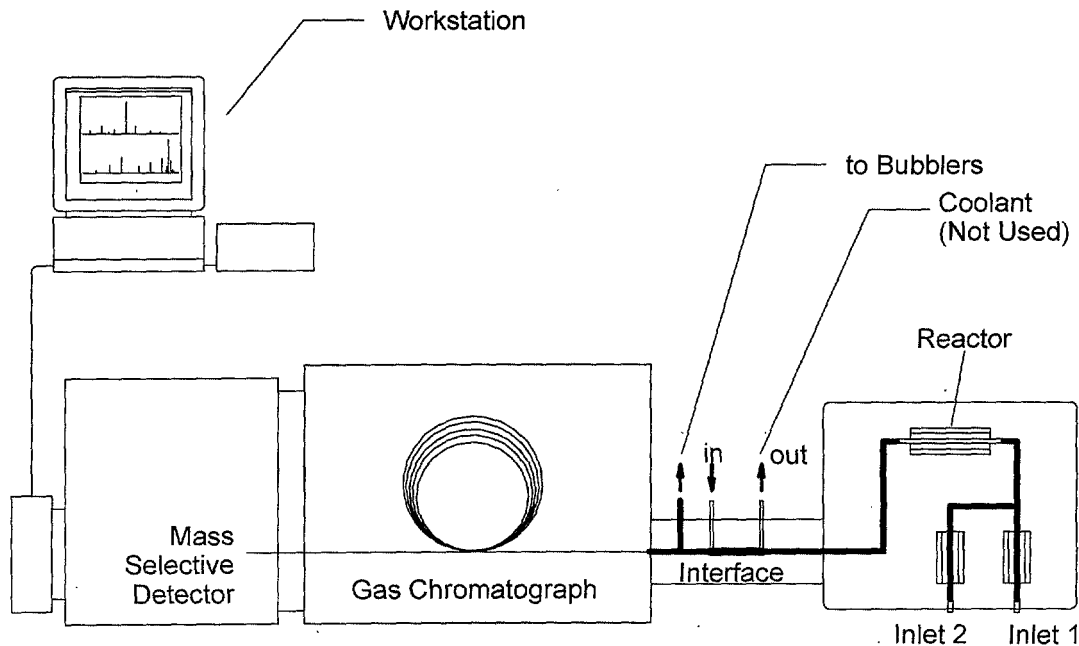

1 The ATRS consists of a reactor assembly and in-line gas
2 chromatograph/detector system connected via an interface.
3 The reactor assembly consists of a thermally insulated
4 enclosure housing the sample introduction, reactor, and
5 transfer line systems.

6
7 Sample introduction for solid materials (Inlet 1) employs a
8 pyroprobe, a device designed to gasify samples by heating
9 them at a fixed rate. The main gas flow will also be fed
10 via Inlet 1, and Inlet 2 will be used to feed supplemental
11 flow.

12
13 During combustion tests, the transfer line between the
14 pyroprobe and the reactor is heated and maintained above
15 200 °C. The reactor is housed within its own small tube
16 furnace and may be independently heated to as high as 1100
17 °C. (Actual conditions for this test program are presented
18 in Section C.2.4.3.) The transfer line from the reactor to
19 the interface is heat traced to greater than 200 °C to
20 prevent cool regions where reactor products could otherwise
21 be lost through condensation.

22
23 The interface routes the combustion exhaust gas to the in-
24 line gas chromatograph (GC) and mass selective detector
25 (MSD) or to sample collection for off-line analysis. For
26 combustion testing in this test program, the interface will
27 also be maintained above 200 °C. Exhaust gas monitoring for
28 this program is described in Section C.2.4.5.

29 30 C.2.4.3 Combustion Test Experimental Conditions

31
32 Each test substance composite will be subjected to
33 laboratory-scale incineration using the experimental
34 apparatus described in Section C.2.4.2.

35 36 C.2.4.3.1 Combustion Air

37
38 Synthetic air (mixture of 21% oxygen and 79% nitrogen) will
39 be used in place of compressed air to prevent potential
40 interference in the experimental system due to background
41 levels of CO₂ in compressed air.

42 43 C.2.4.3.2 Fuel

44
45 Methanol will be used, as needed, as a supplemental fuel to
46 ensure the presence of sufficient hydrogen to convert

1 fluorine to hydrogen fluoride (HF) and chlorine to hydrogen
2 chloride (HCl).

3
4 As noted in *Municipal Solid Waste in the United States:
5 2000 Facts and Figures* (EPA, 2002), paper and paper
6 products (made from wood) make up the largest component of
7 municipal solid waste (MSW). The sum of paper and paper
8 products with wood in MSW makes up over 30% of MSW.

9
10 During the 19th century, methanol was produced from wood and
11 was known as wood alcohol. Therefore, methanol can be used
12 in this experimental program as a surrogate for the paper
13 and wood fraction of MSW.

14 C.2.4.3.3 Operating Conditions

15
16
17 The target operating conditions for the high temperature
18 reactor during the combustion tests for each test substance
19 composite identified in Appendix A.3 are presented in Table
20 C.2-1.

21
22

TABLE C.2-1. COMBUSTION TEST TARGET OPERATING CONDITIONS

Temperature	1000 °C
Residence Time	2 sec
O ₂ concentration in exhaust gas	10%
H ₂ O concentration in exhaust gas	15%
Number of replicate runs	3

23
24 These conditions are conservatively representative of
25 typical furnace operating conditions of municipal waste
26 combustors (MWCs) and of typical secondary chamber
27 operating temperatures for medical waste incinerators in
28 the U.S. See Appendix D.4 for supporting information.

29
30 Temperature and residence time values in Table C.2-2 will
31 be fixed setpoints for these experiments. The temperature
32 of the high temperature reactor will be controlled within
33 ± 10 °C to assure isothermal operation.

34
35 The amount of each test substance composite fed to the ATRS
36 in this testing program will be a measured amount less than
37 5 mg. The actual amount fed, gasification rate (determined
38 from TGA), air supply, and fuel supply will be adjusted to
39 assure that the oxygen level in the exhaust will be greater
40 than or equal to the concentration in Table C.2-1
41 throughout each test to be representative of typical MWC
42 conditions. The fuel supply and air supply will also be

1 adjusted as needed to approach the target H₂O concentration
2 in exhaust gas in Table C.2-1.

3
4 The pyroprobe section final temperature (at end of
5 temperature ramp-up) will be 750 °C or as needed to assure
6 this section is 50 to 100 °C above the highest temperature
7 for complete gasification across the test substance
8 composites as determined from the TGA results; see Section
9 C.2.3. This is necessary to assure complete gasification
10 of the sample of test substance composite and a common set
11 of experimental conditions across the test materials during
12 combustion testing.

13 14 C.2.4.3.4 Blanks

15
16 A minimum of one thermal blank will be run prior to each
17 set of three combustion test runs for a given test
18 substance composite. Each thermal blank run will be at the
19 corresponding combustion test conditions with all feeds
20 except for the test substance.

21 22 C.2.4.4 Process Monitoring

23
24 ATRS process parameters in Table C.2-2 will be monitored
25 for each combustion test at key points during the test as
26 noted in the table. Each combustion test will be a minimum
27 of 5 minutes in duration. If the duration of a combustion
28 test is greater than 15 minutes, each parameter in Table
29 C.2-2 will be recorded at least once every 15 minutes.

30
31 **TABLE C.2-2. COMBUSTION TEST MONITORING**

Parameter	Key Time for Recording
Temperature-Reactor	Before & after gasification
Temperature-Transfer line	Before & after gasification
Temperature-Inlet 1	After gasification
Temperature-Inlet 2	Before & after gasification
Gas flow rate-Inlet 1	Before & after gasification
Gas flow rate-Inlet 2	Before & after gasification
Total Gas Flow rate	Before & after combustion test
Make-up Gas (He) Flow rate	Before & after combustion test
Pressure-Reactor	Before & after gasification

32
33 Temperature-Inlet 1 will be recorded at the end of the
34 temperature ramp-up for gasification to monitor the
35 pyroprobe final temperature.

36

1 The flow rate of the exhaust gas routed to the bubblers
2 (see Section C.2.4.5.2) will be determined based on the
3 flow measurements listed in Table C.2-2.

4
5 The amount of material fed to the system will be verified
6 by weighing the pyroprobe insert cartridge before and after
7 each experiment.

8
9 Exhaust gas monitoring is described in Section C.2.4.5.

10 11 C.2.4.5 Exhaust Gas Monitoring

12
13 Combustion exhaust gas will be continuously monitored for
14 oxygen during each combustion test via in-line MSD or via
15 an oxygen monitor. CO₂ in exhaust gas will be monitored via
16 in-line GC, in-line MSD, or a continuous monitor; or
17 exhaust gas will be collected in Tedlar® bags for off-line
18 analysis of CO₂. Carbon monoxide (CO) in exhaust gas will
19 be monitored via in-line GC or a continuous monitor; or
20 exhaust gas will be collected in Tedlar® bags for off-line
21 analysis of CO. Tedlar® bag samples may be collected at
22 the exit of the bubblers described in Section C.2.4.6.

23 24 C.2.4.6 Exhaust Gas Sampling

25
26 Gas samples for off-line analysis will be collected as
27 described in Appendix D.1, revised as necessary pursuant to
28 Appendix C.1.2.2 if applicable.

29
30 A minimum of 60 mL of bubbler aqueous solution composite is
31 expected from each combustion test. Of this, a minimum of
32 45 mL will be directed to PFOA analysis, and the remainder
33 will be directed to fluoride ion analysis.

34 35 C.2.4.7 Exhaust Gas Analysis

36 37 C.2.4.7.1 Fluoride Ion

38
39 A portion of the composite bubbler aqueous solution sample
40 from each combustion test collected as described in Section
41 C.2.4.6 will be analyzed for fluoride ion via ion
42 chromatography using EPA Method 300.0.

43 44 C.2.4.7.2 PFOA

45
46 A portion of the composite bubbler aqueous solution sample
47 from each combustion test collected as described in Section

1 C.2.4.6 will be analyzed for PFOA via LC/MS/MS as described
2 in Appendix D.2.

3
4 As described in Appendix D.2, composite bubbler aqueous
5 solution sample results less than method detection limit
6 (MDL) will be reported as not detected (ND), results
7 between MDL and the limit of quantitation (LOQ) will be
8 reported as not quantifiable (NQ), and numerical values
9 will not be reported.

10
11 Due to background levels of PFOA, the analytical laboratory
12 will only report numerical values for PFOA concentration in
13 the aqueous solution greater than or equal to the LOQ.
14 This is required to assure that the reported concentration
15 value is attributable to the aqueous solution sample rather
16 than to background.

17
18 C.2.5 Reporting of Results

19
20 C.2.5.1 Elemental Analysis Results

21
22 The results of elemental analysis for each test substance
23 composite (as noted in Section C.2.1) will be reported.
24 The laboratory reports will be included in an appendix to
25 the final report for incineration testing (test report).

26
27 C.2.5.2 Combustion Stoichiometry Results

28
29 Combustion stoichiometry (as noted in Section C.2.2)
30 calculations for each test substance composite will be
31 included in an appendix to the test report.

32
33 C.2.5.3 TGA Results

34
35 The temperature for complete gasification and the TGA
36 graphical results for each test substance composite (as
37 noted in Section C.2.3) will be included in an appendix to
38 the test report.

39
40 C.2.5.4 Combustion Test Results

41
42 C.2.5.4.1 Process Monitoring

43
44 Process monitoring data (as noted in Section C.2.4.4)
45 recorded for each combustion test will be reported in
46 tabular form.

47

1 C.2.5.4.2 Exhaust Gas Monitoring

2

3 Exhaust gas O₂, CO and CO₂ monitoring results will be
4 reported as the integrated or average value for each
5 combustion test. CO will be reported in terms of parts per
6 million by volume (ppmv). O₂ and CO₂ will be reported in
7 terms of percent by volume (%).

8

9 C.2.5.4.3 Exhaust Gas Analytical Results

10

11 Results of analyses noted in Section C.2.4.7 will be
12 reported for each replicate of each combustion test.

13

14 The analytical result for each analyte in Section C.2.4.7
15 will be reported in terms of concentration (mass per
16 volume) in the bubbler aqueous solution. For each analyte,
17 this value will be used with the associated exhaust gas
18 volume to compute an exhaust gas concentration and with the
19 associated test substance mass to compute mass of analyte
20 per mass of test substance composite.

21

22 C.2.5.4.3.1 Fluoride

23

24 Fluoride ion in the exhaust gas will be reported on the
25 basis of mass of fluoride ion per mass of test substance
26 composite. The corresponding hydrogen fluoride value for
27 each will also be computed and reported for reference.

28

29 C.2.5.4.3.2 PFOA

30

31 PFOA results for the bubbler aqueous solution samples will
32 be reported as described in Section C.2.4.7.2. PFOA
33 results for associated blanks will also be reported.

34

35 If present in the bubbler aqueous solution at a
36 concentration above the matrix-specific LOQ, PFOA in the
37 exhaust gas will be reported on the basis of mass of PFOA
38 per mass of test substance composite.

39

40 C.2.5.5 Release Assessment

41

42 In the event that PFOA is reported for the exhaust gas
43 bubbler aqueous solution at a concentration at or above the
44 LOQ (as defined in Appendix D.2) for two or more of the
45 three runs for a given test substance composite, a release
46 assessment report for the full-scale waste incineration of
47 products represented by the test substance composite will

1 be prepared following the outline in Appendix E.2 and will
2 be included in the test report.

3

4 C.2.5.6 Test Report Outline

5

6 The outline for the test report is presented in Appendix
7 E.3. All reporting discussed in Sections C.2.5.1 through
8 C.2.5.5 will be included in this test report, as
9 applicable.

1 **APPENDIX D.1**
2 **EXHAUST GAS SAMPLING VIA BUBBLERS**

3
4 Gas samples for off-line analysis will be collected from a
5 vent line off the interface of the thermal reactor system
6 described in Appendix C.2.4. Flexible (silicone or
7 equivalent) tubing will connect the vent line and a set of
8 bubblers.

9
10 Gas absorption via these bubblers will provide aqueous
11 solution (of documented content) to analyze for prescribed
12 parameters. Two to four bubblers (low pressure drop
13 impingers) in series will be used. Each bubbler will
14 contain a predetermined amount of aqueous solution, and the
15 total amount of solution at the beginning of each test run
16 will be a minimum of 55 mL. The temperature of the gas
17 exiting the last bubbler will be monitored.

18
19 An additional bubbler (which is empty) will be added to the
20 front end of this series of bubblers to serve as a knock-
21 out pot if calculations or preliminary measurements
22 indicate that greater than 10 mL of water will be produced
23 during the testing for a given material.

24
25 Upon completion of sample collection, the amount in each
26 bubbler will be weighed and recorded, and the contents of
27 the bubblers will be composited for subsequent analysis.
28 Additionally, the flexible tubing will be rinsed with 5 mL
29 of HPLC water to collect potential condensate in the
30 tubing; this rinsate will be combined with the bubbler
31 composite prior to analysis.

32
33 Bubbler aqueous solution composites will be conveyed to
34 analytical laboratory(ies) in polyethylene, polypropylene,
35 or glass container(s).

APPENDIX D.2**PFOA ANALYSIS BY LC/MS/MS**

D.2.1 Introduction

Samples to be analyzed for PFOA in this study will be subjected to Liquid Chromatography with Tandem Mass Spectrometry (LC/MS/MS) in accordance with "Method of Analysis for the Determination of Ammonium Perfluorooctanoate (APFO) in Water Revision 1" (Exygen method) revised per the section-by-section comments listed in Section D.2.4 below. These revisions are necessary to adapt a method originally developed for liter quantity water samples to samples related to testing described in Appendix C.

The testing programs described in Appendix C are expected to generate samples of aqueous solution, methanol (e.g., as used for extraction or rinsing), and corresponding blanks. The expected sample size for aqueous solution samples (from exhaust gas bubbler sample collection) available for analysis via this method is approximately 50 mL.

D.2.2 Method Summary

PFOA is extracted from water using a disposable C₁₈ solid phase extraction (SPE) cartridge. PFOA is eluted from the cartridge with methanol. Quantification of PFOA is accomplished by electrospray liquid chromatography/tandem mass spectrometry (LC/MS/MS) analysis.

D.2.3 Reporting

The target limit of quantitation (LOQ) for this study with this method is 50 ng/L based on prior work with water samples where an 8-fold concentration via extraction using C₁₈ SPE cartridge has been demonstrated. The actual LOQ will be matrix dependent; for samples (e.g., methanol rinsate) where the 8-fold concentration cannot be performed, the target LOQ for this study is 400 ng/L.

Sections 4.5.4 and 5 of the Exygen method explain reporting for field samples such as bubbler aqueous solution composites, which are distinct from blanks and spikes, as follows:

Field samples in which either no peaks or peaks

1 less than the MDL are detected at the corresponding
2 analyte retention time will be reported as ND (not
3 detected). Samples in which peaks are detected at
4 the corresponding analyte retention time that are
5 less than the LOQ and greater than or equal to the
6 MDL will be reported as NQ (not quantifiable).

7
8 Therefore, sample results less than method detection limit
9 (MDL) will be reported as ND, and sample results between
10 MDL and the limit of quantitation (LOQ) will be reported as
11 NQ. Numerical values will not be reported for such
12 samples. Only concentrations above the LOQ, where the
13 reported concentration is attributable to the sample rather
14 than to background, are reported with numerical values.

15
16 Additionally, if the PFOA anion is found in a sample at a
17 concentration above the LOQ for the matrix but is less than
18 5 times the concentration found in the associated blank,
19 the result will be flagged and treated as ND.

20
21 D.2.4 Study-Specific Comments on the Method
22

Section	Comment
1	<ul style="list-style-type: none"> • The concentration of PFOA found will be reported directly and the mathematical conversion for reporting as APFO mentioned in the 4th sentence of the 2nd paragraph will not be performed. • Since the 8-fold concentration described in the 2nd sentence 4th paragraph (which forms the basis for the LOQ in the 3rd paragraph and the MDL in the 4th paragraph) is dependent on having a minimum of 40 mL of aqueous sample amenable to extraction using the C₁₈ SPE cartridge described in section 4.4 of the method, the LOQ and MDL in the method will be a factor of 8 higher than reported where less than 40 mL of sample is available or where the sample is not amenable to extraction using the C₁₈ SPE cartridge described in section 4.4 of the method (e.g., methanol).
3.3 Note at top of page 8	<ul style="list-style-type: none"> • The note stating "Equivalent materials may be substituted for those specified in this method if they can be shown to produce satisfactory results" will not be used in the analysis for this testing program.

3.3 Notes, Note 1	<ul style="list-style-type: none"> The following text will be used in place of Note 1 with respect to the PFOA analysis conducted for this testing program: In order to avoid contamination, the use of disposable labware (tubes, pipets, etc.) is required.
3.3 Notes, Note 4	<ul style="list-style-type: none"> The following text will be used in place of Note 4 with respect to the PFOA analysis conducted for this testing program: Solvents (e.g., methanol) used for this analysis must be checked for the presence of contaminants by LC/MS/MS before use.
3.5 opening text prior to 3.5.1	<ul style="list-style-type: none"> Where the available amount of sample is expected to be much less than 1 liter, insufficient sample is available to prepare the fortified matrix spikes described in the opening text of section 3.5. In this case, the analytical standards discussed in this opening text will be limited to two purposes since the third purpose (matrix spike) stated in the method cannot be done.
4.3, item b	<ul style="list-style-type: none"> Where the available amount of sample is expected to be less than 80 mL ($= 2 * 40$), the replicate extraction noted in the first sentence of this item cannot be performed. If the sample is not an aqueous sample amenable to extraction using the C₁₈ SPE cartridge described in section 4.4 of the method, then section 4.4 is skipped such that the sample is analyzed directly. (Note: For such samples, the LOQ and MDL will be 8 times higher than the values quoted in the method.)
4.3, item c	<ul style="list-style-type: none"> As noted in comment on section 3.5 opening text above, fortified matrix spikes will not be prepared when the available amount of sample is much less than 1 liter. Where the available amount of sample is expected to be less than 80 mL ($= 2 * 40$), the conditional repeat fortification and extraction described in the third sentence of this item cannot be performed.
4.4	<ul style="list-style-type: none"> Extraction using the C₁₈ SPE cartridge requires a suitable aqueous sample. This extraction and the corresponding 8-fold concentration

	pointed out in the NOTE at the end of this section cannot be performed on non-aqueous (e.g., methanol) samples.
4.4, item 1	<ul style="list-style-type: none"> In order to measure out the 40 mL mentioned in this item, it is necessary to have at least 45 mL of sample to enable pipet transfer.
4.5.4, item g	<ul style="list-style-type: none"> A storage stability study for PFOA in water performed independently of the development of the method indicates that PFOA may be stored in glass, polystyrene, polypropylene, or polyethylene containers without measurable degradation for up to 68 days prior to extraction. Therefore, the total holding time between sample collection and analysis for aqueous PFOA samples in this study may exceed the 14 day limit noted in the first sentence of this item provided that the sample is not held for greater than 68 days unless additional storage stability testing justifies a longer hold time.
4.6, item 3	<ul style="list-style-type: none"> As noted in comment on section 3.5 opening text above, fortified matrix spikes will not be prepared when the available amount of sample is much less than 1 liter. In this case, acceptance criteria for matrix spike recoveries will not be considered.
5, item c	<ul style="list-style-type: none"> The calculation in equation 3 in this section will not be performed since it is not necessary to convert the PFOA analytical results to APFO for this study.

1

2

D.2.5 Reference

3

4

Flaherty, J. and K. Risha, "Method of Analysis for the

5

Determination of Ammonium Perfluorooctanoate (APFO) in

6

Water Revision 1", Exygen Method No. 01M-008-046 Revision

7

1, January 2003. (EPA Docket ID OPPT-2003-0012-0040)

1 **APPENDIX D.3**
2 **WICKBOLD TORCH METHOD FOR TOTAL FLUORINE**


3
4 D.3.1 Introduction

5
6 "The carbon-fluorine bond is exceptionally strong, and
7 extremely vigorous conditions are needed for quantitative"
8 analysis of fluorine in organic compounds. (Kissa, 1998)
9 The "most vigorous" technique for measurement of fluorine
10 in organic compounds is "combustion in an oxyhydrogen
11 flame" referred to as the Wickbold torch. (Kissa, 1998)

12
13 D.3.2 Apparatus

14
15 A typical configuration for the Wickbold oxyhydrogen torch
16 apparatus as described by Sweetser (1956) is shown in
17 Figure D.3-1.

18
19
20 **FIGURE D.3-1. WICKBOLD OXYHYDROGEN TORCH APPARATUS**

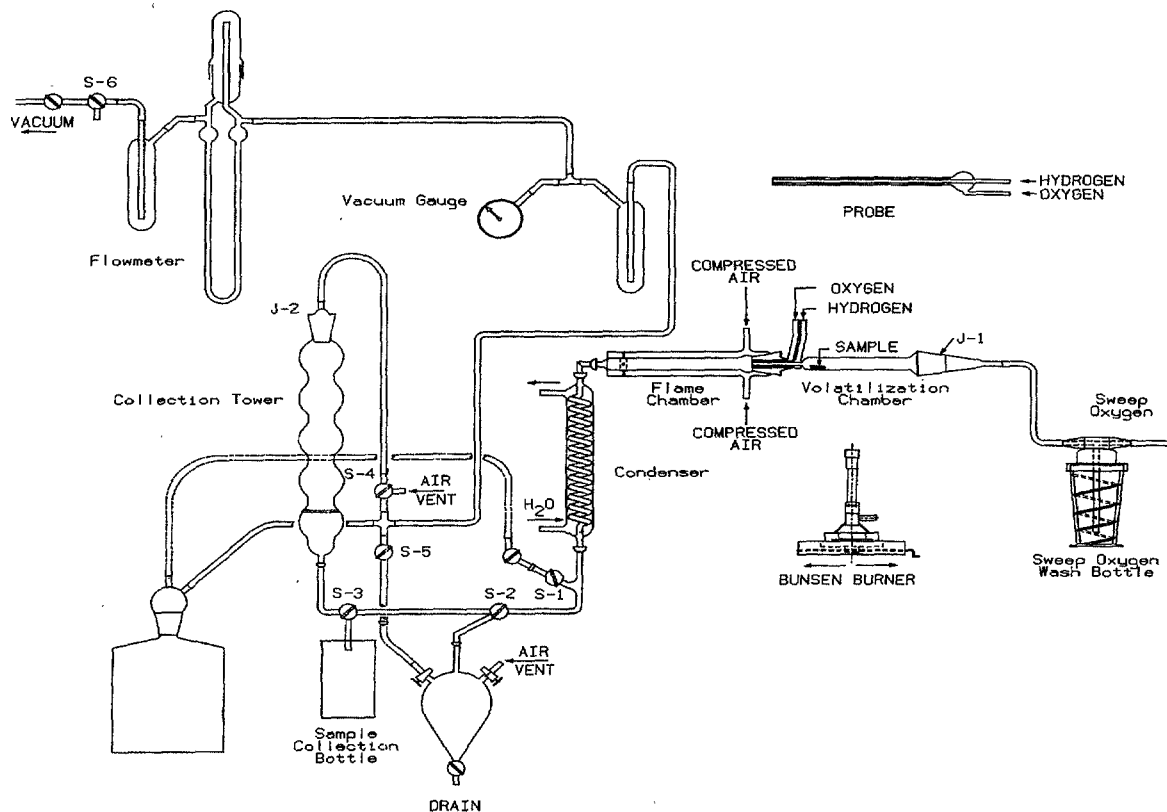

1 D.3.3 Method Description

2

3 The sample size for the standard sample boat is up to 20 mg
4 for a solid or up to 5 mL for a liquid.

5

6 With the oxyhydrogen torch in operation, the sample is
7 pyrolyzed or vaporized with a Bunsen burner moving on a
8 rail below the volatilization chamber. The vapors and
9 pyrolysis products are swept through the oxygen-hydrogen
10 flame chamber operating at up to approximately 2000 °C to
11 mineralize the fluorine in the sample to fluoride ion. The
12 resulting fluoride ion is absorbed in the collection tower
13 containing water or an alkaline solution.

14

15 The absorbed fluoride ion is measured via fluoride ion-
16 selective electrode or ion chromatography.

17

18 The reported limit of quantitation for total fluorine via
19 the Wickbold Torch method is 0.5 ppm (0.5 mg/kg). The
20 accuracy of this method for determination of total fluorine
21 in fluorinated polymers is exemplified by total fluorine
22 values of 75.35% to 75.84% for PTFE with known total
23 fluorine content of 76.0%. (Sweetser, 1956)

24

25 D.3.4 Safety Considerations

26

27 Use of hydrogen presents a potential fire and explosion
28 hazard. Use of oxygen presents a potential fire hazard.
29 Safe operation of the oxyhydrogen torch is assured by the
30 use of specialized equipment with shielding and elaborate
31 safety devices by well-trained personnel at a qualified
32 laboratory.

33

34 D.3.5 References

35

36 Kissa, E. "Analysis of Anionic Fluorinated Surfactants",
37 Chapter 8 in Anionic Surfactants: Analytical Chemistry -
38 2nd Edition, Revised and Expanded, edited by John Cross.
39 Marcel Dekker Surfactant Science Series, volume 73, 1998.

40

41 Sweetser, P. B. "Decomposition of Organic Fluorine
42 Compounds by Wickbold Oxyhydrogen Flame Combustion Method",
43 Analytical Chemistry, vol. 28, pp. 1766-1768, 1956.

1 **APENDIX D.4**
2 **WASTE INCINERATION AND OPERATION CONDITIONS**

3
4 Polymers of the sort being investigated in this testing
5 program may be present at trace to low concentrations in
6 the feedstreams to municipal waste combustors and/or
7 medical waste incinerators in the U.S.

8
9 **D.4.1 Types of Incinerators**

10
11 D.4.2.1 Municipal Waste Combustors

12
13 According to the Integrated Waste Services Association
14 (IWSA), there are a total of 98 waste-to-energy facilities
15 operating municipal waste combustors (MWCs) in the U.S. as
16 of 2002. (IWSA 2002) Table D.4-1 summarizes the number and
17 annual capacity of these units by type of technology
18 employed.

19
20 **Table D.4-1. MWCs in 2002**

Type	Number of Facilities	Annual Capacity (million Ton/year)	Fraction of Waste
Mass Burn	68	22.5	76.5%
Refused Derived Fuel (RDF)	18	6.4	21.8%
Modular	12	0.5	1.7%
Total	98	29.4	100.0%

21
22 D.4.1.2 Hospital/Medical/Infectious Waste Incinerators

23
24 Although earlier reports indicated approximately 2400
25 medical waste incinerators in the U.S. in the 1990s burning
26 approximately 846 thousand tons of hospital and
27 medical/infectious waste (EPA 1997), the current EPA Office
28 of Air Quality, Planning, and Standards (OAQPS) inventory
29 indicates that there are 116 hospital/medical/infectious
30 waste incinerators (HMIWIs) in the U.S. as of July 28,
31 2003. (EPA 2003)

32
33 This represents a greater than 90% reduction in the number
34 of operating HMIWIs in the U.S. Many medical waste
35 incinerators were closed rather than upgraded to meet new
36 emission standards, as hospitals improved their programs to
37 segregate infectious ("red bag") waste burned in HMIWIs
38 from non-infectious ("black bag") waste handled as
39 municipal solid waste after it leaves the hospital.
40 Consequently, the amount of segregated infectious waste

1 burned in HMIWIs is expected to be less than 0.3 million
2 tons per year.

3
4 EPA notes that over 97% of medical waste incinerators are
5 controlled air modular units (EPA 2000a). Recent
6 communication with EPA OAQPS indicates that virtually all
7 existing HMIWIs are controlled air modular (two-chamber)
8 units.

9 10 **D.4.2 Incinerator Operating Conditions**

11
12 Many incinerators for municipal solid waste are designed to
13 operate in the combustion zone at 1800 °F (982 °C) to 2000
14 °F (1093 °C) to ensure good combustion. (EPA 1995) EPA's
15 new source performance standards (NSPS) and emission
16 guidelines for both municipal waste combustors (MWCs) and
17 hospital/medical/infectious waste incinerators (HMIWIs) are
18 based on the use of "good combustion practices" (GCP). (EPA
19 1997, EPA 2000b, EPA 2000c, Van Remmen 1998)

20
21 Referring to MWCs, Donnelly notes, "Design of modern
22 efficient combustors is such that there is adequate
23 turbulence in the flue gas to ensure good mixing, a high-
24 temperature zone (greater than 1000 °C) to complete burnout,
25 and long enough residence time at high temperature (1-2
26 sec) for complete burnout." (Donnelly 2000) The term "flue
27 gas" here refers to the gas above the grate.

28
29 With respect to HMIWIs, Van Remmen states "any unit which
30 presently [prior to compliance date] has a [secondary
31 chamber] residence time less than two seconds at 1000 °C
32 does not meet the requirement for good combustion under the
33 new regulations." (Van Remmen 1998)

34
35 Similarly, most MWCs operate with a 2 second gas residence
36 time in the high temperature zone in order to assure
37 compliance with emission standards on carbon monoxide (CO)
38 and dioxins.

39 40 **D.4.2.1 MWC Operating Conditions**

41 42 **D.4.2.1.1 Mass Burn MWC**

43
44 Review of the IWSA Directory (IWSA 2002) indicates that
45 almost all of these mass burn units are mass burn water
46 wall furnaces. Nearly all mass burn water wall furnaces

1 have reciprocating grates or roller grates to move the
2 waste through the combustion chamber. (EPA 1996a)

3
4 Studies on the Millbury, Massachusetts mass burn water wall
5 MWC produced gas temperature versus residence time results.
6 (Scavuzzo, Strempek, and Strach 1990) Calculations based
7 on Figure 6 of this paper indicate a time-averaged
8 temperature of 2238 °F (1226 °C) over a 2 second. The
9 corresponding gas temperature at the 2 second level from
10 this figure is 1750 °F (954 °C).

11
12 A report on the Warren County, New Jersey mass burn water
13 wall MWC indicates that the design gas temperature between
14 the grate and secondary air inject was greater than 2000 °F
15 (1093 °C) over a gas residence time of an additional 2.2
16 seconds. (Schuetzenduebel and Nobles 1990) This report
17 also shows that this MWC was designed for 2 seconds
18 residence time above 1800 °F (982 °C) between the
19 introduction of secondary air and the exit of the furnace
20 section. (Schuetzenduebel and Nobles 1990) The temperature
21 profile (Figure 21) in the temperature correlation test
22 report (Schuetzenduebel 1989) for this MWC shows the full
23 load gas temperature at the secondary air injection point
24 is 2650 °F, and the gas temperature at the 2-second point is
25 1850 °F. Therefore, testing indicates an average
26 temperature of 2250 °F (1232 °C) over this 2 second gas
27 residence time for the Warren County unit. A related
28 report for the Warren County MWC by the design firm
29 indicates that the exhaust gas oxygen concentration is
30 nominally 10% (dry basis). (Blount Energy Resource Corp.
31 1989)

32
33 Information from these 2 MWCs demonstrates that the average
34 gas temperature across a 2 second residence time for mass
35 burn MWCs is conservatively expected to be greater than
36 1100 °C.

37
38 Test report data from a typical mass burn MWC (Fairfax,
39 Virginia) indicates typical average furnace exit gas
40 concentrations are 10.8% oxygen (dry basis) and 18.4%
41 moisture (water). (Clean Air Engineering, 1997)

42
43 As indicated in Table D.4.1, mass burn units account for
44 over 76% of the municipal solid waste incinerated in the
45 U.S.

1
2 D.4.2.1.2 RDF MWC
3

4 Furnace temperatures as well as flue gas oxygen and moisture
5 (H₂O) levels for the Mid-Connecticut RDF combustor during
6 performance tests while operating under good combustion
7 conditions across a range of steam loads (Finklestein and
8 Klicius 1994) are summarized in Table D.4-2.
9

10 **Table D.4-2. RDF MWC - Mid-Connecticut**

Steam load	low	low	inter- mediate	inter- mediate	normal	normal	normal	high
test number	PT-13	PT-14	PT-10	PT-02	PT-09	PT-08	PT-11	PT-12
Furnace temperature (°C)	965	1004	1012	1022	1033	1015	1026	1049
flue gas O ₂ (%)	10.1	9.6	9.2	9.1	7.6	7.5	7.9	6.4
flue gas moisture	12.4	11.1	12.3	15.4	15.1	16.3	14.1	16.2

11
12 The average operating conditions for this RDF unit across
13 the range of steam loads are 1016 °C, 8.4% O₂ (dry basis),
14 and 14.1% moisture.
15

16 Examination of the report and MWC temperature monitoring
17 practices indicates that these temperatures are effectively
18 combustion zone exit temperatures. Therefore, in order to
19 determine the average MWC combustion zone temperature
20 across a 2 second gas residence time, it is necessary to
21 understand the time-temperature profile of the MWC.
22

23 Since waste combustion in this and most other RDF units in
24 the U.S. involves burning on the grate (EPA 1996a) similar
25 to the operation of mass burn MWCs, the time-temperature
26 profile in an RDF unit is expected to be similar to that
27 described in Section D.4.2.1.1 above. Based on this
28 similarity and the temperatures in Table D.4-2, the average
29 gas temperature across a 2 second residence time for RDF
30 units is conservatively expected to be greater than 1100 °C.
31

32 As indicated in Table D.4.1, RDF units account for
33 approximately 22% of the municipal solid waste incinerated
34 in the U.S.
35

36 D.4.2.1.1 Modular MWC
37

38 Modular MWCs are generally small dual-chamber units,
39 accounting for less than a total of 2% of the municipal
40 solid waste incinerated in the U.S. in 2002. Modular MWCs
41 are generally equipped with auxiliary fuel burners in the

1 secondary chamber. (EPA 1996a) EPA notes that the
2 secondary chamber exit temperature of modular MWCs is
3 maintained at typically 980 to 1200 °C. (EPA 1996a)
4

5 A typical modular MWC in Polk County, Minnesota is operated
6 with a gas residence time of 2 seconds, in the secondary
7 chamber, a secondary chamber exit temperature in the range
8 of 1800 °F (982 °C) to 2000 °F (1093 °C), flue gas oxygen
9 concentrations in the range of 10% to 13% (dry basis), and
10 flue gas moisture in the range of 10% to 15% (Pace
11 Analytical 2003).
12

13 Since the secondary chamber exit temperature is expected to
14 be the minimum gas-phase temperature for the chamber, the
15 secondary chamber average gas temperatures for modular MWCs
16 are expected to be 1000 °C or greater.
17

18 As indicated in section D.4.1, such modular units are
19 generally small MWCs and account for less than a total of
20 2% of the municipal solid waste incinerated in the U.S.
21

22 D.4.2.1.4 MWC Summary 23

24 Considering the relative quantities of municipal waste
25 burned annually in each type of MWC and the data in this
26 section, typical operating conditions for the high
27 temperature zone of most MWCs are >1000 °C average
28 temperature across 2 second residence time with exit gas
29 concentrations of 10% O₂ (dry basis) and >15% moisture.
30

31 D.4.2.2 HMIWI Operating Conditions 32

33 The range of temperatures for the secondary chamber of
34 controlled air medical waste incinerators has been reported
35 as 980 to 1200 °C. (Theodore 1990) EPA notes that auxiliary
36 fuel (e.g., natural gas) is burned in the secondary chamber
37 of medical waste incinerators to sustain temperatures in
38 the range of 985 to 1095 °C and that combustion air at 150
39 to 250 % of the stoichiometric requirement is usually added
40 to the secondary chamber. (EPA 2000a, EPA 1994a)
41

42 In its model plant description background document, EPA
43 notes that the average moisture content in HMIWI flue gas
44 was about 10 % based on available data, and EPA states
45 "limited data show that older [HMIWI] units typically have
46 residence times that range from essentially 0 seconds up to
47 about 1 second." (EPA 1994b) However, as noted above, a

1 more recent report indicates that HMIWIs still in operation
2 have secondary chamber temperatures greater than or equal
3 to 1000 °C with a gas residence time of 2 seconds. (Van
4 Remmen 1998) For example, EPA studied the incinerator at
5 Weeks Hospital in New Hampshire as a typical HMIWI with a
6 design residence time of 2 seconds in the secondary
7 chamber. (EPA 1996b) During this testing, the average exit
8 secondary chamber exit temperature was 1024 °C, and the flue
9 gas oxygen concentration was 13.5%. (dry basis) (EPA 1996b)

10
11 Review of test reports for all HMIWIs in the EPA docket for
12 the HMIWI NSPS and EG rulemakings that are listed in EPA's
13 current HMIWI inventory (EPA 2003) does not refute Van
14 Remmen's statement above on residence time and temperature
15 and indicates HMIWI flue gas oxygen concentrations for
16 these units in the range of 10 to 15% (dry basis) and stack
17 moisture concentrations as high as 30% (after wet
18 scrubbing). (Environmental Laboratories Inc. 1993, EPA
19 1996, HDR Engineering 1994a, HDR Engineering 1994b, METCO
20 Environmental 1992, Technical Services, Inc. 1993,
21 Technical Services, Inc. 1994a, Technical Services, Inc.
22 1994b) Apparently, the older HMIWIs referred to in EPA's
23 model plant description background document either have
24 been shut down or upgraded to operate with secondary
25 chamber exit temperatures higher than 1000 °C at a gas
26 residence time of 2 seconds.

27
28 Secondary chamber temperature of HMIWIs is monitored near
29 the secondary chamber outlet. (EPA 1994) Hence, when the
30 auxiliary burner (located on the end opposite from the
31 outlet) is in use, the average gas temperature in an HMIWI
32 secondary chamber is greater than the outlet temperatures
33 noted above. Therefore, secondary chamber average gas
34 temperatures for HMIWIs are expected to be 1000 °C or
35 greater with a gas residence time of 2 seconds.

36
37 In summary, typical operating conditions for the secondary
38 chamber of operating HMIWIs in the U.S. are 1000 °C average
39 temperature across 2 second residence time with exit gas
40 concentrations of 13% O₂ (dry basis) and >10% moisture.

41 42 **D.4.3 Pollution Control Equipment**

43
44 Over 99% of large MWC capacity operates with a spray dryer
45 absorber/scrubber. (IWSA 2003) Approximately 80% of large
46 MWC capacity operates using carbon injection as part of the
47 pollution control system. (IWSA 2003) Due to requirements

1 in the NSPS (EPA 2000b) and EG (EPA 200c) for small MWCs,
2 small MWCs planning continued operation are generally
3 upgrading or have upgraded their pollution control
4 equipment to add spray dryer absorbers or other acid gas
5 control and carbon injection.

6
7 Review of EPA's HMIWI inventory (EPA 2003) indicates that
8 essentially all HMIWIs have some form of wet or dry
9 scrubbing for acid gas control.

10

11 **D.4.4 Summary**

12

13 Approximately 30 million tons per year of municipal solid
14 waste was combusted in the United States annually in waste-
15 to-energy municipal waste combustors in 2003.

16 Approximately 0.3 million tons per year of segregated
17 medical waste was combusted annually in the United States
18 in hospital/medical/infectious waste incinerators in 2003.
19 Considering the relative amounts of waste combusted
20 annually, typical operating conditions for waste
21 incineration in the U.S. across these two classes of units
22 are as follows:

23

Average Temperature	>1000 °C
Residence Time	≥2 sec
O ₂ concentration in exhaust gas	10% (dry basis)
H ₂ O concentration in exhaust gas	15%

24

25 EPA emission regulations currently in place or in place by
26 2005 require that operating municipal waste combustors and
27 hospital/medical/infectious waste incinerators have or will
28 have air pollution control equipment such as wet or dry
29 scrubbing for acid gas control.

30

1 **References**

- 2
- 3 Blount Energy Resource Corp. Correlation Procedure for
4 Continuously Monitoring Furnace Temperatures (Warren County
5 Resource Recovery Facility), March 22, 1989.
- 6
- 7 Clean Air Engineering. Test Report for Covanta of Fairfax,
8 Inc. I-95 Energy/Resource Recovery Facility, 1997.
- 9
- 10 Donnelly, J.R. Waste Incineration Sources: Municipal Waste
11 Combustion. In: W.T., ed., Air Pollution Engineering
12 Manual, 2nd edition. Air and Waste Management Association.
13 New York, NY: Van Nostrand Reinhold, 2000, pp 257-268.
- 14
- 15 Environmental Laboratories Inc. Stack Test Report for
16 Emissions Testing of the Bethesda Memorial Hospital Waste
17 Incinerator, Boynton Beach Florida, September 13, 1993.
- 18
- 19 Environmental Protection Agency (EPA). Municipal Waste
20 Combustion Assessment: Technical Basis for Good Combustion
21 Practice, EPA 600/8-89-063, August 1989.
- 22
- 23 EPA. Medical Waste Incinerators - Background Information
24 for Proposed Standards and Guidelines: Control Technology
25 Performance Report for New and Existing Facilities, EPA-
26 453/R-94-044a, July 1994.
- 27
- 28 EPA. Medical Waste Incinerators - Background Information
29 for Proposed Standards and Guidelines: Model Plant
30 Description and Cost Report for New and Existing
31 Facilities, EPA-453/R-94-045a, July 1994.
- 32
- 33 EPA. Decision Maker's Guide to Solid Waste Management,
34 Volume II, Chapter 8, 1995.
- 35
- 36 EPA. AP-42, Fifth Edition, Volume I, Chapter 2: Solid
37 Waste Disposal, Section 2.1, Refuse Combustion, Supplement
38 B, October 1996.
- 39
- 40 EPA. Medical Waste Incineration Emission Test Report:
41 Weeks Memorial Hospital, Lancaster, New Hampshire, EMC
42 Report 96-MWI-11, March 1996.
- 43
- 44 EPA. Standards of Performance for New Stationary Sources
45 and Emission Guidelines for Existing Sources:
46 Hospital/Medical/Infectious Waste Incinerators, 62 Federal
47 Register 48346, September 15, 1997.

1
2 EPA. Exposure and Human Health Reassessment of 2,3,7,8-
3 Tetrachlorodibenzo-p-Dioxin (TCDD) and Related Compounds,
4 Part I: Estimating Exposure to Dioxin-Like Compounds Volume
5 2: Sources of Dioxin-Like Compounds in the United States,
6 Chapter 3, EPA/600/P-00/001Bb, Draft Final Report,
7 September 2000.
8
9 EPA. New Source Performance Standards for New Small
10 Municipal Waste Combustion Units, 65 Federal Register
11 76350, December 6, 2000.
12
13 EPA. Emission Guidelines for Existing Small Municipal
14 Waste Combustion Units, 65 Federal Register 76378, December
15 6, 2000.
16
17 EPA. HMIWI Facility and Emissions Inventory, draft, July
18 28, 2003,
19 www.epa.gov/ttnatw01/129/hmiwi/2003hmiwi_inventory.xls
20
21 Finklestein, A. and R. D. Klicius. National Incinerator
22 Testing and Evaluation Program: The Environmental
23 Characterization of Refuse-derived Fuel (RDF) Combustion
24 Technology, Mid-Connecticut Facility, Hartford,
25 Connecticut, EPA-600/R-94-140 (NTIS PB96-153432), December
26 1994.
27
28 HDR Engineering. Performance Test Results Report
29 Submittal: Incinerator Waste Management Facility, Mayo
30 Foundation, Rochester, Minnesota, June 7, 1994.
31
32 HDR Engineering. Performance Test Results Report
33 Supplemental Submittal Charts, Data Sheets, Operator Log,
34 CEMS Data: Incinerator Waste Management Facility, Mayo
35 Foundation, Rochester, Minnesota, June 10, 1994.
36
37 Integrated Waste Services Association (IWSA). The 2002
38 IWSA Directory of Waste-to-Energy Plants, 2002,
39 www.wte.org/2002_directory/IWSA_2002_Directory.html
40
41 IWSA. Air Pollution Control Devices on Operating Waste-to-
42 Energy Plants: Year 2002, 2003.
43
44 METCO Environmental. Source Emissions Survey of University
45 of Texas Medical Branch, Incinerator Number 2 Exhaust Duct,
46 Galveston, Texas, TACB Permit C-18655 for Clever Brooks,
47 July 1992.

1
2 Midwest Research Institute. Updated Hospital/Medical/
3 Infectious Waste Incinerator Inventories Received from
4 Various Regions, States, and Counties, January 27, 1999.
5
6 Pace Analytical. Comprehensive Emissions Test Report: MSW
7 Incinerator Unit No. 1 ESP Outlet & MSW Incinerator Unit
8 No. 2 ESP Outlet (Polk County Solid Waste Plant), March 11-
9 14, 2003.
10
11 Scavuzzo, S. A., J. R. Strempek, and L. Strach. "The
12 Determination of the Thermal Operating Characteristics in
13 the Furnace of a Refuse-Fired Power Boiler" in Proceedings
14 of the 1990 National Waste Processing Conference, American
15 Society of Mechanical Engineers (ASME), 1990, pp. 397-404.
16
17 Schuetzenduebel, W. G. and W. C. Nobles. "New Jersey's
18 First Resource Recovery Facility (The Warren County Energy
19 Recovery Facility)" in Proceedings of the 1990 National
20 Waste Processing Conference, ASME, 1990, pp. 321-343.
21
22 Schuetzenduebel, W. G. Blount Energy Corporation Report -
23 Furnace/Boiler Temperature Correlation: Warren County
24 Resource Recovery Facility, Oxford, New Jersey, October
25 1989.
26
27 Technical Services, Inc. Source Test Report: Boca Raton
28 Hospital, Boca Raton, Florida, March 31-April 2, 1993.
29
30 Technical Services, Inc. Source Test Report: Mercy
31 Hospital South Miami, Florida, July 27-28, 1994.
32
33 Technical Services, Inc. Source Test Report: St. Vincent's
34 Medical Center Jacksonville, Florida, August 30, 1994.
35
36 Theodore, L. Air Pollution Control and Waste Incineration
37 for Hospitals and Other Medical Facilities, Van Nostrand
38 Reinhold, New York, 1990, pp 313-320.
39
40 Van Remmen, T. Evaluation of the available air pollution
41 control technologies for achievement of the MACT
42 requirements in the newly implemented new source
43 performance standards (NSPS) and emission guidelines (EG)
44 for hospital and medical/infectious waste incinerators,
45 Waste Management, 1998, Vol. 18, pp 393-402.
46

1 **APPENDIX E.1**
2 **OUTLINE FOR INTERIM PROGRESS REPORTING**
3
4

5 Title: Enforceable Consent Agreement for the Laboratory-
6 Scale Incineration Testing of Fluorotelomer Based
7 Polymers - Interim Report
8

9 OPPT Docket ID No: OPPT-2004-0001

10
11 Date of Interim Report: [date]
12
13
14

15 This Report covers the period from [date] to [date]
16
17

18 1) List or description of significant ECA Test Program
19 milestones during this period:
20
21
22
23
24

25 2) Description of Difficulties: (If none indicate N/A)
26
27
28
29
30
31
32

33 3) Actions taken in response to difficulties: If none
34 indicate N/A
35
36
37
38
39
40

41 4) Other information relevant to the progress of the
42 testing program: (If none indicate N/A)
43

1 **APPENDIX E.1 (continued)**2 **OUTLINE FOR INTERIM PROGRESS REPORTING**

3

4

5 Title: Enforceable Consent Agreement for the Laboratory-
6 Scale Incineration Testing of Fluoropolymers -
7 Interim Report

8

9 OPPT Docket ID No: OPPT-2003-0071

10

11 Date of Interim Report: [date]

12

13

14

15 This Report covers the period from [date] to [date]

16

17

18 1) List or description of significant ECA Test Program
19 milestones during this period:

20

21

22

23

24

25 2) Description of Difficulties: (If none indicate N/A)

26

27

28

29

30

31

32

33 3) Actions taken in response to difficulties: If none
34 indicate N/A)

35

36

37

38

39

40

41 4) Other information relevant to the progress of the
42 testing program: (If none indicate N/A)

1 **APPENDIX E.2**
2 **OUTLINE FOR RELEASE ASSESSMENT REPORT**
3

4 As described in Appendix C.2.5.5 of this ECA, if PFOA is
5 reported for the exhaust gas bubbler aqueous solution at a
6 concentration at or above the LOQ (as defined in Appendix
7 D.2) for two or more of the three runs for a given test
8 substance composite, then the potential for release from
9 full-scale municipal and/or medical waste incineration, as
10 applicable, (including application of air pollution
11 controls) of products represented by the test substance
12 composite in the United States will be assessed to put the
13 data into perspective. At a minimum, the report will
14 follow the general outline described below and will state
15 assumptions, document the basis for the assumptions made,
16 quantitatively estimate the variability of calculated
17 estimates (based on the variability of the parameters in
18 the evaluation), and qualitatively discuss the uncertainty
19 of calculated estimates.

20
21 **1.0 Introduction**
22

- 23 • Statement of objective for combustion testing of
24 test substance composites.
25
26 • Applicability of the laboratory-scale combustion
27 testing to full-scale municipal waste combustors
28 (MWCs) and/or medical waste incinerators (as
29 applicable) in the United States.
30

31 **2.0 Summary of study results**
32

- 33 • A listing of exhaust gas analytical results reported
34 for each applicable test substance composite.
35
36 • A listing of test substance composite analytical
37 results reported for each applicable test substance
38 composite.
39

40 **3.0 Discussion**
41

- 42 • Description of the combustion section of the
43 applicable waste incineration process(es) being
44 evaluated (MWC and/or medical waste incinerator)
45 including the rationale for selecting test target
46 temperature(s) and description of typical

1 operational parameters. Cross-reference to or
2 submission of relevant parts of Appendix D.4 of this
3 ECA can satisfy this provision.
4

- 5 • Description of the post-combustion air pollution
6 control equipment (e.g., lime scrubbing, carbon
7 adsorption) employed by typical operating full-scale
8 waste incineration process(es) as applicable.
9

10 **4.0 Extrapolation of laboratory test results to the**
11 **typical waste incineration process(es), as applicable,**
12 **described in Section 3.0 (above) for each test**
13 **substance composite to be evaluated.**
14

- 15 • The relevance of the subject test substance
16 composite to MWCs and/or medical waste incinerators.
17
- 18 • The estimated concentration of the subject test
19 substance composite to the applicable type(s) of
20 waste incinerator. Available information on
21 hydrogen fluoride concentration in waste incinerator
22 exhaust can provide the basis for an upper bound on
23 this estimated concentration.
24
- 25 • A description of the extrapolation.
26
- 27 • A description of any assumptions used.
28
- 29 • Any unique qualitative or quantitative descriptors
30 of the test, the testing equipment, and the results
31 deemed necessary for informative review of the test
32 and test results.
33

34 **5.0 Sensitivity Analysis**
35

- 36 • Assessment of the impact of variability
37 (quantitative) and uncertainty (qualitative) in each
38 parameter on the evaluation results.
39

40 **6.0 Conclusions**
41

42 **7.0 References**

1 **APPENDIX E.3**2 **OUTLINE OF TEST REPORT****

3

4

5 Table of Contents

6

7 Executive Summary

8

9 Introduction

10

11 I. Phase I PFOA Transport Testing

12

13 1. Experimental Apparatus

14 2. Description of Test Conditions (including deviations
15 from protocol)

16 3. Documentation of PFOA Standard

17 4. Analytical Results

18 4.1 PFOA

19 4.2 Total Fluorine

20 5. Transport Efficiency

21 5.1 PFOA

22 5.2 Total Fluorine

23 6. Discussion of Results

24 7. Conclusions

25

26 II. Phase II Incineration Testing (provided Phase II is performed)

27

28 1. Documentation of Test Substance Composites

29 2. Elemental Analysis Results

30 3. Combustion Stoichiometry Results

31 4. TGA Results

32 5. Combustion Testing

33 5.1 Experimental Apparatus

34 5.2 Description of Test Conditions (including deviations
35 from protocol)

36 5.3 Combustion Testing Results

37 5.3.1 Process Monitoring

38 5.3.2 Exhaust Gas Monitoring

39 5.3.2 Exhaust Gas Sampling and Analysis

40 5.3.2.1 PFOA

41 5.3.2.2 Fluoride

42 5.4 Discussion of Results

43 5.5 Conclusions

44

45 III. Appendices

46

- 47 • Quality Assurance Report(s)

- 1
2 • Report(s) from Compositing Facility(ies) (provided Phase II
3 is performed)
4
5 • Reports from Analytical Laboratories
6
7 • Release Assessment per Appendix E.2, if applicable
8
9
10
11 * Test Report will include this information (as applicable)
12 but not necessarily in this format.
13
14 ** References to literature in this report will include full
15 citations.

1 **APPENDIX F**
 2 **ECA INCINERATION TESTING QUALITY ASSURANCE PROJECT PLAN (QAPP):**
 3 **REQUIRED CONTENT**
 4

EPA QA/R-5 QAPP Guidance Element	Required Content of QAPP(s) for ECA Incineration Testing
A: PROJECT MANAGEMENT	
A1 Title and Approval Sheet	to be included in QAPP
A2 Table of Contents	to be included in QAPP
A3 Distribution List	to be included in QAPP
A4 Project/Task Organization	to be included in QAPP
A5 Problem Definition/ Background	to be satisfied by cross-reference to ECA (Parts I, IV) and Appendix A, C.1, or C.2, as applicable
A6 Project/Task Description	see element A5
A7 Quality Objectives and Criteria	to be satisfied by cross-reference to Appendix A, C.1, or C.2 (as applicable) and to Appendix D.2 and/or D.3, as applicable
A8 Special Training/ Certifications	for facilities subject to GLP (40 CFR Part 792) under this ECA, QAPP shall state that this element is satisfied by compliance with applicable GLP requirements; for compositing facilities, to be to be satisfied by providing a statement of the qualifications for each such facility
A9 Documentation and Records	to be satisfied by cross-reference to ECA Part XIV and Appendix E
B: DATA GENERATION AND ACQUISITION	
B1 Sampling Process Design (Experimental Design)	see element A5
B2 Sampling Methods	to be satisfied by cross-reference to Appendix C.1 or C.2 (as applicable) and to Appendix D.1
B3 Sample Handling and Custody	to be included in QAPP consistent with Appendix A
B4 Analytical Methods	to be satisfied by cross-

	reference to analytical method descriptions in Appendices C.2, D.2, and D.3, as applicable
B5 Quality Control	to be satisfied by cross-reference to QC provisions (e.g., blanks) in Appendices A, C.1, C.2, D.2, and D.3, as applicable
B6 Instrument/Equipment Testing, Inspection, and Maintenance	to be included in QAPP in summary form for chemical analysis equipment for the analytical methods for element B4 above
B7 Instrument/Equipment Calibration and Frequency	to be included in QAPP in summary form for chemical analysis equipment for the analytical methods for element B4 above
B8 Inspection/Acceptance of Supplies and Consumables	for facilities subject to GLP (40 CFR Part 792) under this ECA, QAPP shall state that this element is satisfied by compliance with applicable GLP requirements; not applicable to other facilities
B9 Non-direct Measurements	to be satisfied by cross-reference to Appendix C.2.2
B10 Data Management	for facilities subject to GLP (40 CFR Part 792) under this ECA, QAPP shall state that this element is satisfied by compliance with applicable GLP requirements; for compositing facilities, to be to be satisfied by cross-reference to Appendix A.4
C: ASSESSMENT AND OVERSIGHT	
C1 Assessments and Response Actions	for facilities subject to GLP (40 CFR Part 792) under this ECA, QAPP shall state that this element is satisfied by compliance

	with applicable GLP requirements; for other facilities, to be included in QAPP
C2 Reports to Management	for facilities subject to GLP (40 CFR Part 792) under this ECA, QAPP shall state that this element is satisfied by compliance with applicable GLP requirements; for other facilities, to be included in QAPP
D: DATA VALIDATION AND USABILITY	
D1 Data Review, Verification, and Validation	to be satisfied by cross-reference to Appendix A, C.1, or C.2 (as applicable) and to Appendix D.2 and/or D.3, as applicable
D2 Verification and Validation Methods	for facilities subject to GLP (40 CFR Part 792) under this ECA, QAPP shall state that this element is satisfied by compliance with applicable GLP requirements; for other facilities, to be included in QAPP consistent with Appendices A, C.1, C.2, D.2, D.3 as applicable
D3 Reconciliation with User Requirements	to be satisfied by cross-reference to Appendices C.2.5.5 and E.2, as applicable

1

1 **APPENDIX G**
2 **COPY OF EPA ORDER**

3
4
5 **UNITED STATES**
6 **ENVIRONMENTAL PROTECTION AGENCY**

7
8 **TESTING CONSENT ORDER FOR THE LABORATORY-SCALE INCINERATION**
9 **TESTING OF FLUOROTELOMER BASED POLYMERS**

10
11 **Docket No. OPPT-2004-0001**

12
13
14 Under the authority of section 4 of the Toxic Substances
15 Control Act (TSCA), 15 U.S.C. 2603, the United States
16 Environmental Protection Agency (EPA) issues this testing
17 consent order (Order) to take effect on the date of publication
18 of the notice in the Federal Register announcing the issuance of
19 this Order. This Order incorporates the enforceable consent
20 agreement (ECA) for the laboratory-scale incineration testing of
21 fluorotelomer based polymer test substance composites listed in
22 Appendix A of the ECA.

23
24
25
26
27
28
29
30
31 _____
Date

32 _____
Stephen L. Johnson,
33 Assistant Administrator
34 For Prevention, Pesticides,
35 And Toxic Substances

1 APPENDIX G (continued)
2 COPY OF EPA ORDER

3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34

UNITED STATES
ENVIRONMENTAL PROTECTION AGENCY

TESTING CONSENT ORDER FOR THE LABORATORY-SCALE INCINERATION
TESTING OF FLUOROPOLYMERS

Docket No. OPPT-2003-0071

Under the authority of section 4 of the Toxic Substances Control Act (TSCA), 15 U.S.C. 2603, the United States Environmental Protection Agency (EPA) issues this testing consent order (Order) to take effect on the date of publication of the notice in the Federal Register announcing the issuance of this Order. This Order incorporates the enforceable consent agreement (ECA) for the laboratory-scale incineration testing of fluoropolymer test substance composites listed in Appendix A of the ECA.

Date

Stephen L. Johnson,
Assistant Administrator
For Prevention, Pesticides,
And Toxic Substances